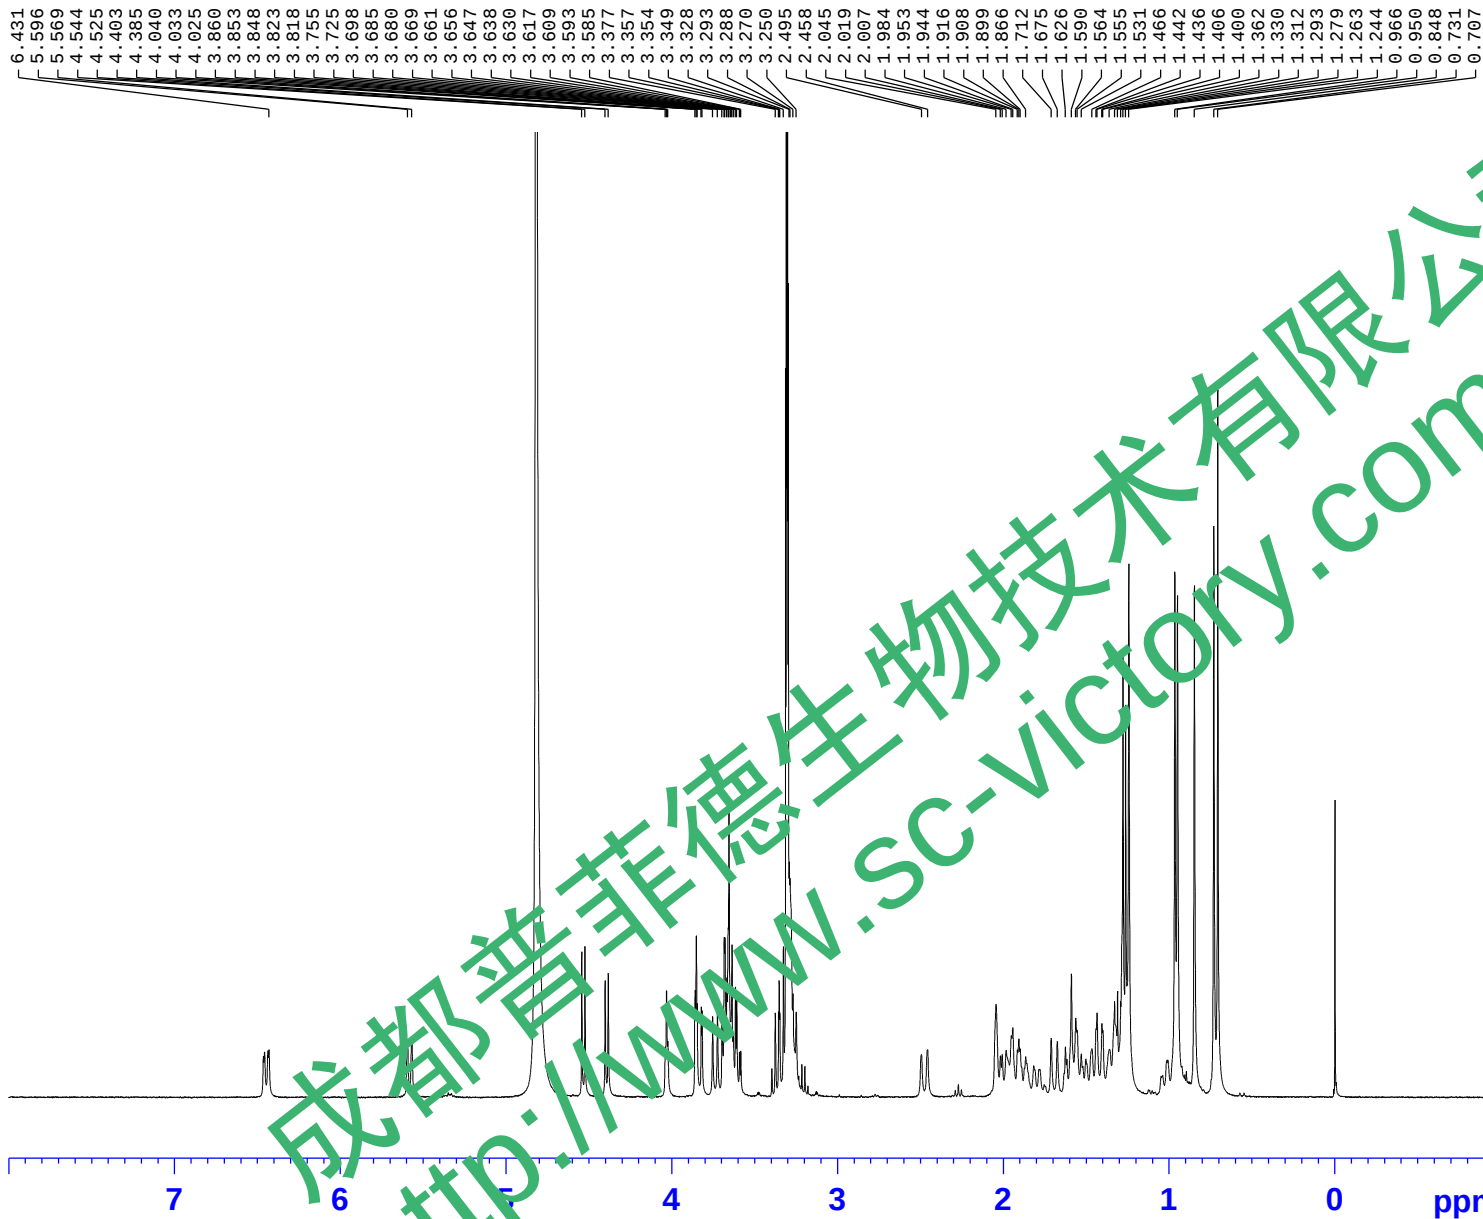


Current Data Parameters  
NAME HuZaoGan B2-1H NMR CD3OD  
EXPNO 1  
PROCNO 1

#### F2 - Acquisition Parameters

INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zg30  
TD 65536  
SOLVENT MeOD  
NS 64  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.122266 Hz  
AQ 4.0894465 sec  
RG 202.5  
DW 62.400 usec  
DE 6.50 usec  
TE 301.2 K  
D1 2.00000000 sec  
TD0 1

===== CHANNEL f1 =====  
SF01 400.1324710 MHz  
NUC1 1H  
P1 14.79 usec  
PLW1 11.50800037 W

F2 - Processing parameters  
SI 65536  
SF 400.1300091 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

— 135.86  
— 131.25  
— 125.67  
— 125.26

104.29  
104.18  
83.80  
82.08  
76.52  
76.32  
73.98  
70.98  
70.49  
69.99  
69.85  
67.70  
63.65  
61.01  
53.45  
46.88  
43.99  
42.62  
41.01  
40.50  
37.98  
37.70  
35.93  
34.42  
31.80  
31.58  
31.50  
30.58  
24.76  
23.91  
23.19  
20.82  
17.70  
17.57  
16.20  
15.56  
11.48



Current Data Parameters  
NAME HuZaoGan B2-13C NMR CD3OD  
EXPNO 1  
PROCNO 1

#### F2 - Acquisition Parameters

INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zgig30  
TD 65536  
SOLVENT MeOD  
NS 2048  
DS 4  
SWH 24038.461 Hz  
FIDRES 0.366798 Hz  
AQ 1.3631488 sec  
RG 202.5  
DW 20.800 usec  
DE 6.50 usec  
TE 301.2 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1

===== CHANNEL f1 =====  
SF01 100.6228298 MHz  
NUC1 13C  
P1 10.13 usec  
PLW1 51.00000000 W

===== CHANNEL f2 =====  
SF02 400.1316005 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 11.50800037 W  
PLW12 0.31077999 W

F2 - Processing parameters  
SI 262144  
SF 100.6127690 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

